




Q-View™ IMAGERPLUS

Operator's Manual

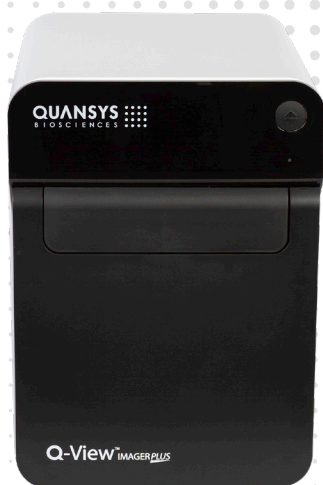

Version 1.1
For Research Use Only
Not For Use in Diagnostic Procedures

Introduction

The Q-View™ Imager Plus is designed to acquire high quality images of chemiluminescent 96-well microtiter plates. It is intended for research use only. Q-View Software™ is intended to be used to control the instrument and for the analysis of data produced by the Q-View Imager Plus.

Notes on Safety

The Q-View Imager Plus has been designed and certified to meet EN61010-1 requirements, which are internationally accepted electrical safety standards. Certified products are safe to use when operated in accordance with the device instruction manual. It is critical that the user read this manual in its entirety and train on the device frequently to ensure proper operation. For laboratory use only, Pollution Degree 2 or better. Recommended for use below 2000 m. If the device is used outside of the instructions herein or modified, disassembled, or altered, the safety of the device cannot be guaranteed. Improper operation will:

1. Void the manufacturer's warranty
2. Void the regulatory certification
3. Create a potential safety hazard

Manual Markings



Indicates a warning: Warnings help prevent safety issues or failures in performance.



Indicates an important notification: Important notifications alert the user to certain steps that are critical for optimal performance.

Notice of Warranty

THIS LIMITED WARRANTY COVERS NORMAL USE. QUANSYS BIOSCIENCES DOES NOT WARRANT AND IS NOT RESPONSIBLE FOR DAMAGES CAUSED BY MISUSE, ABUSE, ACCIDENTS, VIRUSES, UNAUTHORIZED SERVICE OR PARTS, OR THE COMBINATION OF QUANSYS BIOSCIENCES BRANDED PRODUCTS WITH OTHER PRODUCTS. THIS LIMITED WARRANTY DOES NOT COVER NON-QUANSYS BIOSCIENCES BRANDED PRODUCTS. ANY WARRANTY APPLICABLE TO NON-QUANSYS BIOSCIENCES BRANDED SOFTWARE OR PRODUCTS IS PROVIDED BY THE ORIGINAL MANUFACTURER.

Printing History

Version Number:	Date:
1.1	May 2025

Contact Information

Mailing Address:

Quansys Biosciences
365 North 600 West
Logan, Utah 84321

Phone Numbers:

U.S. Toll Free: (888) 782-6797
Direct: (435) 752-0531

Email Addresses:

General Information: info@quansysbio.com
Sales: sales@quansysbio.com
Technical Support: support@quansysbio.com

TABLE OF CONTENTS

Introduction	I
Notes on Safety	I
Manual Markings	I
Notice of Warranty	II
Printing History	II
Contact Information	II
<u>Chapter 1: Installation and Safety Information</u>	3
Safety Precautions	3
Automated Tray	3
Electricity	3
Placement in the Laboratory	4
Temperature and Humidity	4
Ventilation and Dust	4
Space	4
Vibration	5
Q-View Imager Plus Setup	5
Assembly	5
Acquire Dark Field	7
Setup Completion	7
Moving the Q-View Imager Plus	8
Chemical Safety	8
Electronic Considerations	9
Power Cord	9
USB Cord	9
Routine Maintenance	10
Cleaning	10

<u>Chapter 2: System Overview</u>	11
External Features	11
Eject Button	11
LED Status Indicator	11
Back	12
Computer Connection	13
Q-View Software Introduction	13
<u>Chapter 3: Operation</u>	14
Before you Begin	14
Cleaning the Tray Surface	14
Loading the Plate	14
Imaging the Plate	15
Using the Qualification Plate	15
Troubleshooting	16
Troubleshooting Guide:	16
Appendix	17
Q-View Imager Plus Specifications	17
Operating Specifications	17



Manufactured and Distributed by:

Quansys Biosciences

365 North 600 West Logan, Utah 84321, USA

TEL: (888) 782-6797

E-MAIL: info@quansysbio.com

For International Distributors see:

<http://www.quansysbio.com/distributors>



Chapter 1: Installation and Safety Information

SAFETY PRECAUTIONS

Automated Tray



Do not attempt to remove any plates from or insert any plates into the automated tray while the tray is moving. The status LED will turn yellow as the tray opens and strobe until the tray is closed. Only remove or insert plates when the tray is fully extended and is no longer in motion. Any body parts, clothing, or other objects placed in the path of tray travel may be damaged or injured. Upon obstruction of the tray, the indicator light will no longer strobe but remain a solid yellow. Press the plate ejector button to open or close the tray. Do not attempt to close the tray by pushing in on the tray.

Electricity



Since the Q-View Imager Plus has a 110V/220V power supply, exercise typical precautions to ensure shocks do not occur. Do not place liquids close to the Q-View Imager Plus and do not cut cords that provide power or connect the device to the PC.

PLACEMENT IN THE LABORATORY

Temperature and Humidity

The Q-View Imager Plus has 4 high-resolution cameras. If the ambient lab temperature is too high, the cameras may be unable to perform correctly. Recommended operating conditions are 18–27° C. Humidity can also cause operation problems for the Q-View Imager Plus. Ensure your laboratory environment does not exceed a dew point of 17° C to prevent condensation.



NOTE: Q-View Software prevents imaging when the target temperature cannot be reached.

Ventilation and Dust

The fan on the bottom of the device pulls ambient air into the device to cool it. Ensure the room where the Q-View Imager Plus is placed has adequate ventilation to ensure proper cooling. It is important to keep any objects, such as paper or other flat materials, away from the bottom of the Q-View Imager Plus as these can block airflow to the fan. Dust, in high levels, can be pulled into the fan and adhere to the camera cooling apparatus. Dust can also collect on the glass on the tray deck and cause dust particles to be visible in your image. Please take precautions to keep the lab bench surface and floors clean of dust.

Space

The footprint of the Q-View Imager Plus is 24.45 W x 31.75 D x 35.88 H cm (9 5/8 x 12 1/2 x 14 1/8 inches). Ensure the space around the Q-View Imager Plus is free of chemicals that can spill or other equipment that can fall and damage the Q-View Imager Plus.

Vibration

The exposure times of the Q-View Imager Plus can be up to 5 minutes. It's important that the location of the Q-View Imager Plus is free of excessive vibration. Make sure equipment that might cause vibrations such as vortex mixers, shakers, centrifuges, etc. are not located on the bench with the Q-View Imager Plus. Also consider where the Q-View Imager Plus is placed in the laboratory. For example, the Q-View Imager Plus should not be placed on a bench near a door that could be slammed or on a bench near a desk where someone could bump it during image capture.

Q-VIEW IMAGER PLUS SETUP

Assembly

The Q-View Imager Plus weighs approximately 13.6 kg (30 lbs). To correctly set up the Q-View Imager Plus, the following steps should be followed:

1. Place the Q-View Imager Plus in a clean work area. Ensure the location meets the requirements addressed in "Placement in the Laboratory" section above.
2. Connect the power supply to the Q-View Imager Plus.
3. Plug in the wall cord.
4. Install the Q-View Imager Plus Drivers on the computer that will be connected to the imager if you are not using a computer provided by Quansys Biosciences.

5. Connect the USB cord to a USB 3 port on the computer that will be running Q-View™ Software. Using a rear port on the computer is recommended.
6. Turn on the Q-View Imager Plus.
7. Press the plate ejector button to open the tray of the Q-View Imager Plus, ensure the tray where the glass insert fits is free from debris and liquids.
8. Clean the glass insert with a lint-free cloth and 70% ethanol in deionized water, rubbing alcohol, or window cleaner.
9. Place the glass insert in the tray aligning the notch at the top of the insert. The embossed "A" should be in the upper left corner when inserted correctly.
10. Open Q-View Software. The connected imager should automatically be detected and a dialog box should open with a link to Manage Imagers. If this does not occur, in the Settings menu, click Manage Imagers.
11. From the Manage Imagers menu the connected imager may be named and a dark field acquired. If using a computer purchased from Quansys Biosciences, setup is complete at this point.



Acquire Dark Field

Dark Field Image Acquisition minimizes background noise in subsequent plate images. If the Q-View Imager Plus is connected to a computer provided by Quansys Biosciences, Dark Field Acquisition should already be complete and does not need to be repeated. If a Dark Field Image has not been captured, remove any plates from the Q-View Imager Plus, and close the Q-View Imager Plus tray. In the **Settings** menu click on **Manage Imagers**. Select the correct imager and press **Capture Dark Field**. The process will take approximately 35 minutes.

Setup Completion

Once the Q-View Imager Plus setup is finished, the software opens with the **Update Preferences** dialog box. Select your preferences and log in if user accounts are enabled. If your Internet connection on any computer running Q-View Software goes through a proxy, specify these settings under **Administration > Network Settings**. Your Q-View Software and Q-View Imager Plus are now ready to use.

MOVING THE Q-VIEW IMAGER PLUS

Ensure there is no plate on the tray of the Q-View Imager Plus and unplug all cords. The Q-View Imager Plus weighs approximately 13.6 kg (30 lbs).



To move or ship the Q-View Imager Plus, there are several critical steps that should take place.

1. Ensure the new location meets the requirements addressed in "Placement in the Laboratory"
2. Remove any remaining plates on the tray
3. Remove the glass insert
4. Remove all cords from the device
5. Insert the Q-View Imager Plus into the provided plastic sleeve
6. Insert the glass insert into the protective sleeve
7. Bundle and tie cables together
8. Insert the Q-View Imager Plus into the foam insert in the Q-View Imager Plus box
9. Place the glass insert, and cords into the box

CHEMICAL SAFETY

The only chemicals used with the Q-View Imager Plus are deposited within the wells of the plate, which is placed on the glass insert. It is important to take precaution that these chemicals do not spill onto the glass insert. If any spillage occurs on the glass insert, clean it immediately before closing the tray. If liquids are present on the glass insert, they may drip onto the camera lenses and damage the Q-View Imager Plus.



ELECTRONIC CONSIDERATIONS

Power Cord



The power cord is a 3-wire grounding-type plug. This cord will only fit into a grounded outlet, which is a requirement for the Q-View Imager Plus. Do not remove the grounding leg of the plug. Doing so will void all warranties on the Q-View Imager Plus.

The power cord provided with the Q-View Imager Plus is specific to the power supplied in your region. If you have a different voltage supply or need a different power cord for any reason, please contact technical support. Do not use an extension cord for the Q-View Imager Plus. Ensure that all equipment plugged into the same circuit as the Q-View Imager Plus does not exceed the amperes of service, or you may experience a tripped breaker or power failure that could result in the loss of your image.

Before unplugging the power cord, make sure Q-View Software is closed on the PC. Make sure the USB cord is unplugged. At this point, it is safe to remove the power cord.

USB Cord

The USB cord connects the Q-View Imager Plus to the PC, which controls and operates the Q-View Imager Plus. This cord should only be unplugged from the Q-View Imager Plus once Q-View Software is closed.

ROUTINE MAINTENANCE

Cleaning

Cleaning the glass is recommended before every use. Ensure that the glass insert is free from dust and any chemicals. To clean the glass, use 70 percent ethanol or warm water. Do not use scouring cleaners or abrasive pads as this can scratch the glass. Be careful not to spill any cleaning materials inside the Q-View Imager Plus.

The exterior of the device can be cleaned as needed with 70% Ethanol, Rubbing Alcohol, A neutral detergent, or 10% Bleach. Again, be careful not to spill any cleaning materials inside the Q-View Imager Plus.

Regularly Inspect the dust filter located on the bottom of the imager and clean as needed. The dust filter is attached magnetically to the body of the imager. To clean, remove the filter and wipe, wash or blow away accumulated dust. Ensure the filter is clean and dry before reattaching it to the imager.



Regularly inspect all cables for fraying or loose connections.

Chapter 2: System Overview

EXTERNAL FEATURES

Eject Button

There is 1 button on the front of the Q-View Imager Plus. Pressing this button will open and close the imager tray allowing the user to place or remove a plate from the plate holder.



LED Status Indicator


The LED light on the front of the Q-View Imager Plus will change color to indicate the status of the device. The indicator color scheme has been designed to be user friendly for those with normal vision and more common forms of color blindness. The table below is the legend for status light indication.

LED Color		Activity*	Imager Status
White	○	Solid	Startup
White	○	Pulse	Sleep
White	○	Strobe	Firmware update
Magenta (red-purple)	●	Solid	Idle, serial port connected, not software ready
Blue-green	●	Solid	Idle, serial port connected, software ready
Yellow	●	Solid	Tray in motion or open
Yellow	●	Strobe	Tray obstruction
Blue	●	Solid	Plate imaging
Blue	●	Pulse	Transilluminator/focus imaging
Red	●	Solid	Fatal error

*Activity Definitions: Solid - Constant light with no flashing or dimming. Pulse - Slow dimming and brightening of the indicator light. Strobe - Rapid flashing of the light

Back

There are 4 features on the back of the Q-View Imager Plus. An on/off switch, a power plug receptacle, the USB cord receptacle, and a label containing the serial number and power specifications for the unit.

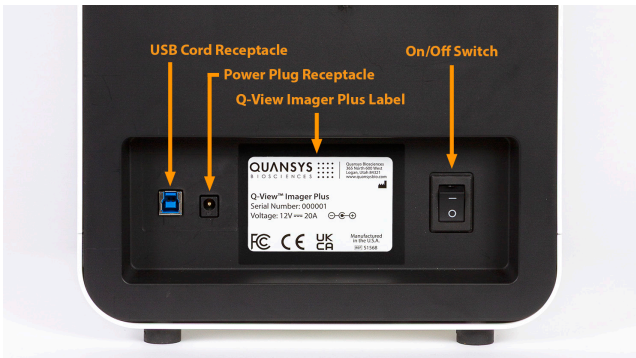


COMPUTER CONNECTION

The Q-View Imager Plus is connected to the PC via a USB 3.0 cable (provided) and should be connected using a USB 3 port. Do not unplug either end of the USB cable without closing Q-View Software on the PC. From within Q-View Software, the user can open Imager Management and see an entry in a table for the Q-View Imager Plus with 1 of the columns saying “connected” or “disconnected.”

Q-VIEW SOFTWARE INTRODUCTION

A copy of Q-View Software will accompany the Q-View Imager Plus. To download and install Q-View Software, request a license key from customer support (sales@quansysbio.com). You may also request a copy of Q-View Software from: quansysbio.com/request-software.

Please contact our technical support staff at support@quansysbio.com for more assistance with Q-View Software.

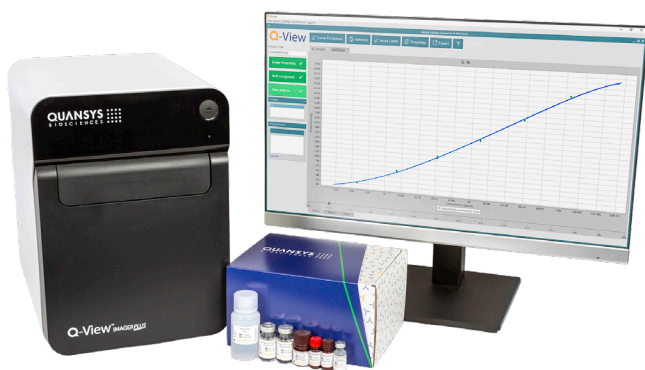

Chapter 3: Operation

BEFORE YOU BEGIN

The following procedure is recommended before every use.

1. Clean the top of the glass insert and ensure it is free of debris.
2. Check within Q-View Software that the Q-View Imager Plus is connected to the PC.

CLEANING THE TRAY SURFACE

If any particulate, liquid, or dried salt residues or smudges are left on the glass or the tray, it will adversely affect the quality of the image and the overall quality of your data. This can be cleaned with 70 percent ethanol in deionized water using a lint-free cloth. Do not use scouring cleaners or abrasive pads as this can scratch the glass.

LOADING THE PLATE

Open the tray by pressing the eject button on the front of the imager. Place the Q-Plex™ plate on the glass insert with well A1 in the top left corner of the tray when facing the imager. Press down gently on the plate to ensure the plate is fully inserted and rests flat on the glass for all bottom edges of the plate. Ensure there is no plate seal on the plate and there is only 1 plate on the tray. Press the eject button to close the tray and proceed to imaging.



IMAGING THE PLATE

In Q-View Software, select **Image Processing** and **Acquire Image**. The name of the connected imager should appear in the dropdown box under **Imager**. If the dropdown says, “No Imagers Connected”, select **Refresh**. The name of the Q-View Imager Plus will appear, and connection can be made.

Select the **Exposure Time** and **Image Name**. Once these settings are made, click on **Capture Image(s)** and Q-View Software will image the plate that has been inserted.

USING THE QUALIFICATION PLATE

The optional Q-View™ Plus Qualification Plate can be used to qualify the performance of the Q-View Imager Plus over time. This plate has varying thicknesses and allows light from the internal transilluminator to be filtered over the range of detection. Parameters can be determined dynamically by the Q-View Software to determine acceptable levels of performance. Due to the sensitivities of the cameras, qualification ranges are built using a particular qualification plate paired with a particular imager. Qualification plates are not transferable to other imagers unless qualification ranges have been built pairing a single qualification plate to multiple imagers.

The qualification plate also contains a barcode sticker to qualify the on-board barcode reader. Do not remove this sticker from the qualification plate.

To establish qualification plate ranges, in the Q-view software go to **Qualification > Q-View Imager Qualification > Settings**, then click on **Build Ranges**. This takes approximately 5 minutes to complete.

To learn more about the Q-View Qualification Plate, please contact Quansys Biosciences sales or technical support.

TROUBLESHOOTING

To resolve any issue with the Q-View Imager Plus, please contact Quansys Biosciences by calling **1-877-QUANSYS (1-877-782-6797)** or send an email describing the issue to support@quansysbio.com. If outside the USA, please contact your Quansys Biosciences distributor for your area. Have your serial number available with a detailed description of the issue. The serial number is located on the label on the back of the device.

TROUBLESHOOTING GUIDE:

Issue	Problem	Solution
Q-View Software is unable to recognize the Q-View Imager Plus	Failure of communication between the Q-View Imager Plus and computer	Ensure power is supplied to the Q-View Imager Plus Ensure the USB cable is connected to both the Q-View Imager Plus and a USB 3 port on the computer Disconnect the Q-View Imager Plus USB cable from the computer and restart the computer
Plate images are blurry	The Q-View Imager Plus is out of focus	Contact Quansys Biosciences for assistance.

Appendix

Q-VIEW IMAGER PLUS SPECIFICATIONS

Resolution:	~35 Megapixels
Pixel Pitch:	1.85 microns
Sensor Type:	CMOS
Sensor Format:	1/1.7
Optics:	Basler C125-1218-5M-P
Image Application:	Chemiluminescent SBS plate format
Imaging Time:	1 second – 300 seconds
Control:	Q-View Software
Connection to PC:	USB 3

OPERATING SPECIFICATIONS

Operating Conditions:	Temperature range of 18-27°C and dew point of no greater than 17°C, non-condensing
Power Requirements:	100-240V AC 50/60Hz 150W
Dimensions:	25.40 W x 29.21 D x 35.56 H cm (10 x 11.5 x 14 inches).
Weight:	13.6 kg (30 lbs)
Overvoltage Category:	OVC II



For technical support, email: support@quansysbio.com

109817GR

365 North 600 West, Logan, Utah 84321
Tel: 1-888-782-6797 | www.quansysbio.com